



2-Blue 3-Red 6-Violet 4-YellGrn new config Nov 2019

Cytometer:	LSRFortessa	User:	Administrator
Cytometer Name:	LSRFortessa	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 9.2
Input Device:	HTS	Date:	5/26/2023 6:54:46 AM
Window Extension:	10.00		


Blue Laser
(488nm)
FSC

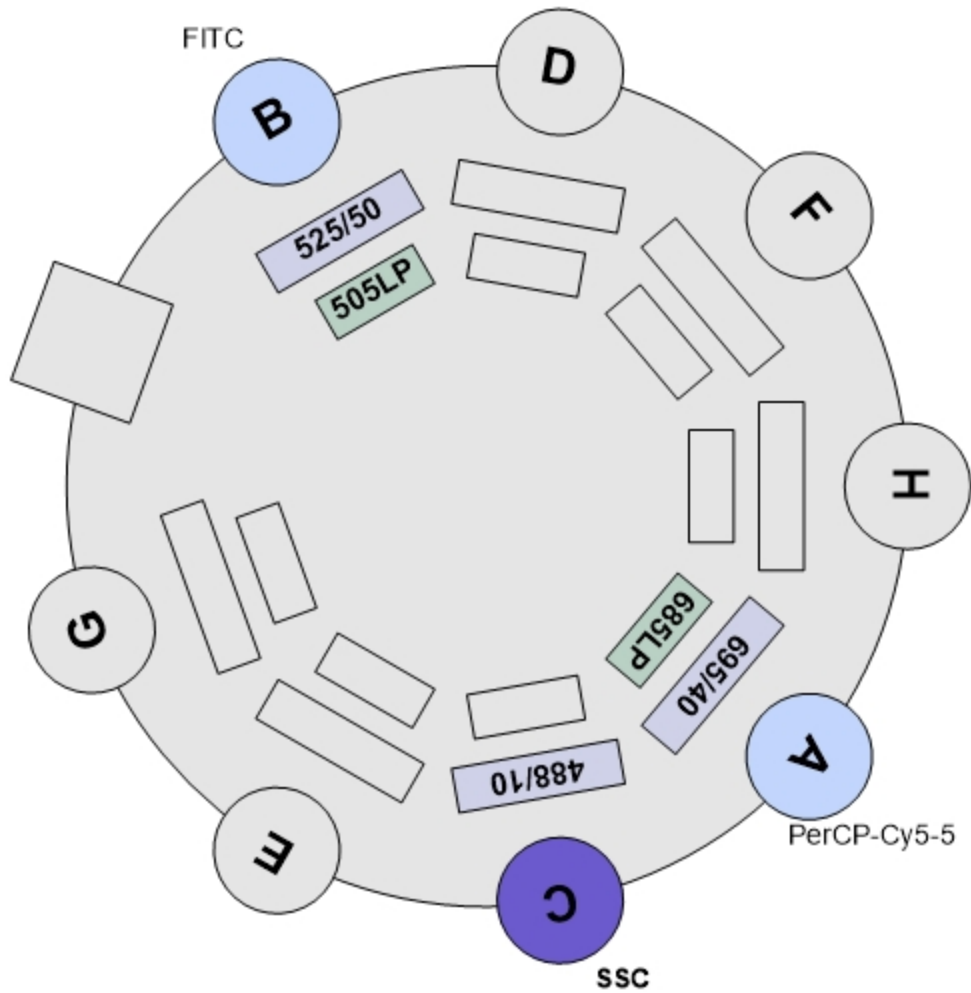


Red Laser
(640nm)

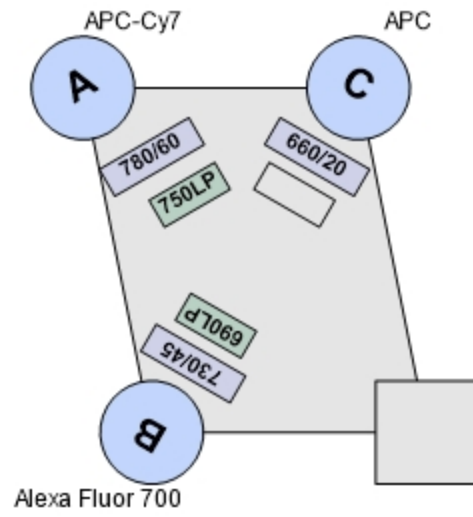

Violet Laser
(405nm)

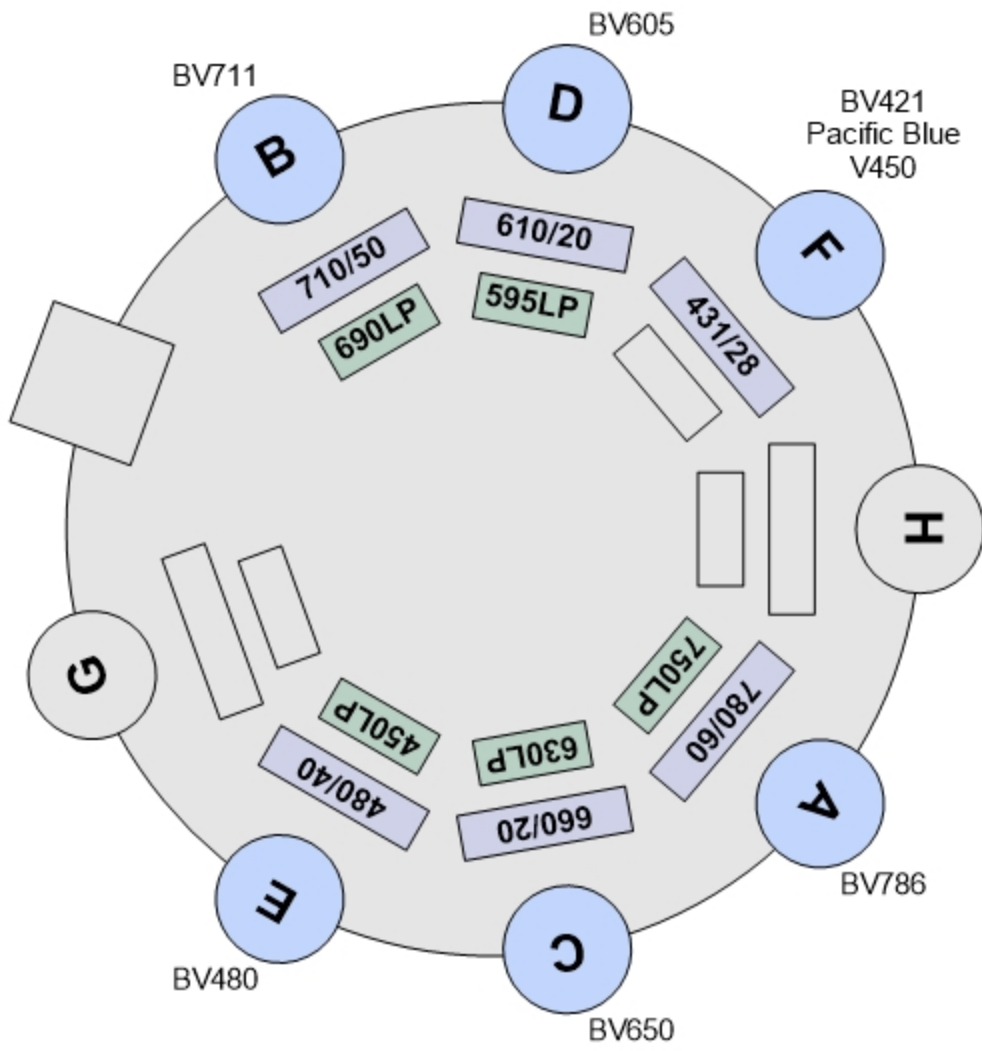

YellGrn Laser
(561nm)

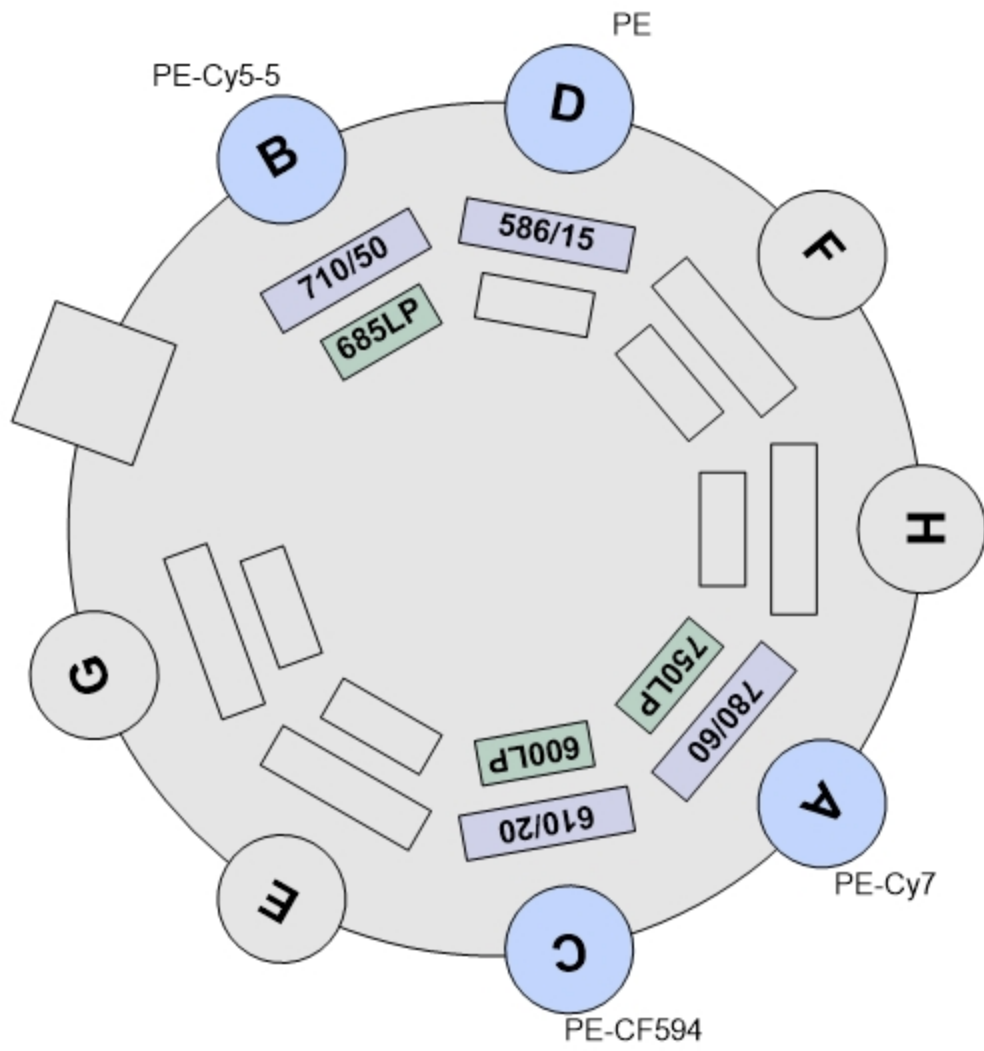

Comments: